


INSTRUCTIONS



No-Wire™ Indexed Rack



+H58818745002310

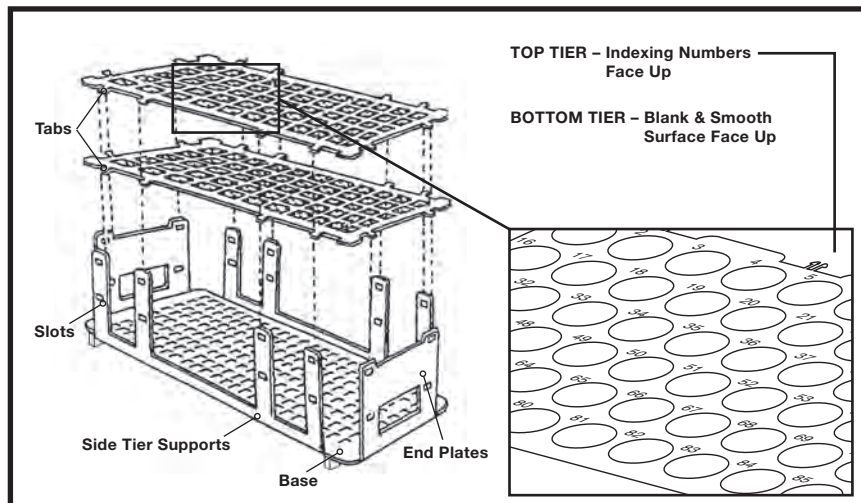

1. Place the base on a flat work surface with the word “BOTTOM” facing down.
2. Bend up one end plate. Snap the bottom tier end tabs into the lower set of slots in the end plate. Be sure the bottom tier imprinted numbers face up.
3. Position the top tier so that imprinted numbers face up and align with the numbers on the bottom tier. Snap the top tier end tabs into the upper set of slots in the end plate.
4. Bend up the opposing end plate and snap the bottom tier and then top tier end tabs into their matching slots in the end plate.

5. Bend up one side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.
6. Bend up the remaining side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.

Submersible and works well in water baths

Autoclavable at 250° F (121°C)

Empty racks can be stacked.

Note: Do not use with liquid nitrogen.

661 Route 23 South, Wayne, NJ 07470



TEL: 973-694-0500 • FAX: 973-694-7199 • www.belart.com

918745017 – 10/15

Bel-Art – SP Scienceware assumes no obligation or liability for any advice furnished by it, or for results obtained with respect to these products.

All such advice is given and accepted at the buyer's risk.

© 2015. All Rights Reserved.

Bel-Art® – SP Scienceware® is a division of SP Industries, Inc.




INSTRUCTIONS



No-Wire™ Indexed Rack



+H58818745002310

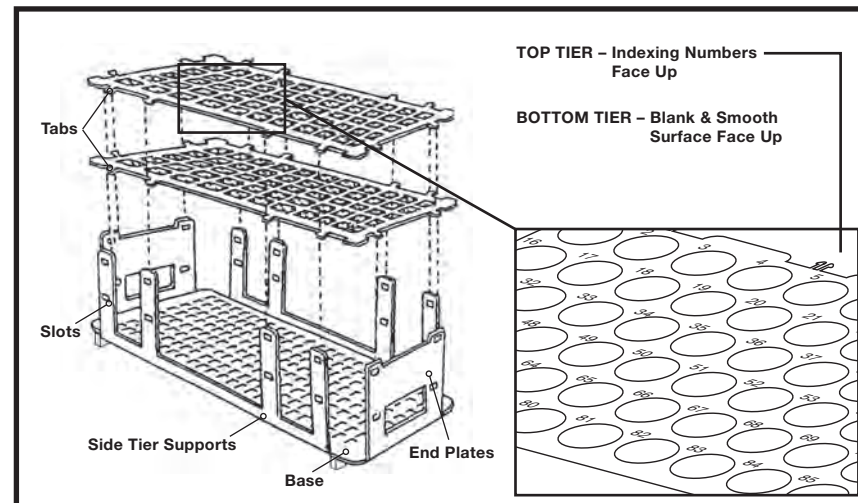

1. Place the base on a flat work surface with the word “BOTTOM” facing down.
2. Bend up one end plate. Snap the bottom tier end tabs into the lower set of slots in the end plate. Be sure the bottom tier imprinted numbers face up.
3. Position the top tier so that imprinted numbers face up and align with the numbers on the bottom tier. Snap the top tier end tabs into the upper set of slots in the end plate.
4. Bend up the opposing end plate and snap the bottom tier and then top tier end tabs into their matching slots in the end plate.

5. Bend up one side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.
6. Bend up the remaining side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.

Submersible and works well in water baths

Autoclavable at 250° F (121°C)

Empty racks can be stacked.

Note: Do not use with liquid nitrogen.

661 Route 23 South, Wayne, NJ 07470



TEL: 973-694-0500 • FAX: 973-694-7199 • www.belart.com

918745017 – 10/15

Bel-Art – SP Scienceware assumes no obligation or liability for any advice furnished by it, or for results obtained with respect to these products.

All such advice is given and accepted at the buyer's risk.

© 2015. All Rights Reserved.

Bel-Art® – SP Scienceware® is a division of SP Industries, Inc.




INSTRUCTIONS



No-Wire™ Serpentine Indexed Rack



+ H 5 8 8 1 8 7 4 5 0 0 9 9 1

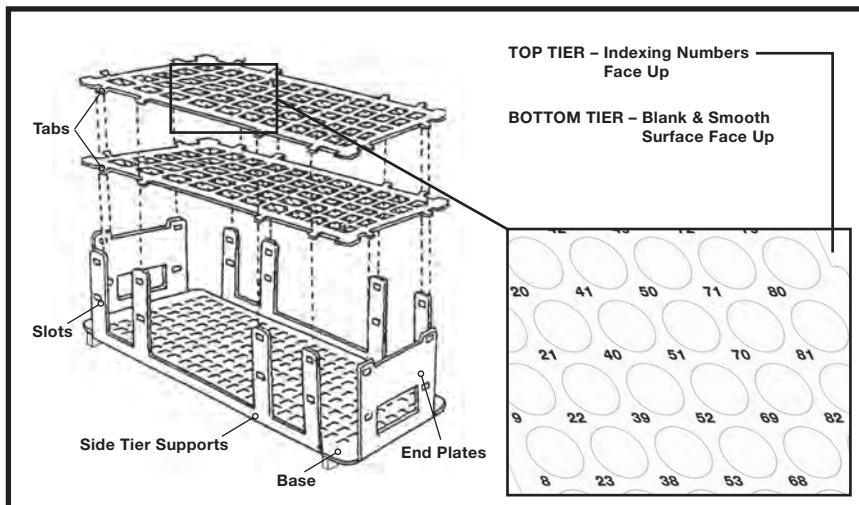

1. Place the base on a flat work surface with the word "BOTTOM" facing down.
2. Bend up one end plate. Snap the bottom tier end tabs into the lower set of slots in the end plate. Be sure the bottom tier imprinted numbers face up.
3. Position the top tier so that imprinted numbers face up and align with the numbers on the bottom tier. Snap the top tier end tabs into the upper set of slots in the end plate.
4. Bend up the opposing end plate and snap the bottom tier and then top tier end tabs into their matching slots in the end plate.

5. Bend up one side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.
6. Bend up the remaining side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.

Submersible and works well in water baths

Autoclavable at 250° F (121°C)

Empty racks can be stacked.

Note: Do not use with liquid nitrogen.

661 Route 23 South, Wayne, NJ 07470



TEL: 973-694-0500 • FAX: 973-694-7199 • www.belart.com

918745022 - 10/15

Bel-Art – SP Scienceware assumes no obligation or liability for any advice furnished by it, or for results obtained with respect to these products.

All such advice is given and accepted at the buyer's risk.

© 2015. All Rights Reserved.

Bel-Art® – SP Scienceware® is a division of SP Industries, Inc.




INSTRUCTIONS



No-Wire™ Serpentine Indexed Rack



+ H 5 8 8 1 8 7 4 5 0 0 9 9 1

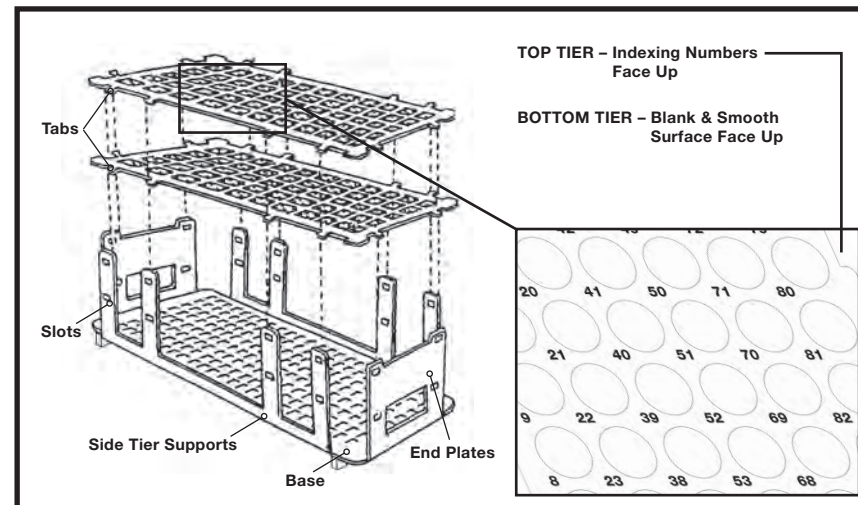

1. Place the base on a flat work surface with the word "BOTTOM" facing down.
2. Bend up one end plate. Snap the bottom tier end tabs into the lower set of slots in the end plate. Be sure the bottom tier imprinted numbers face up.
3. Position the top tier so that imprinted numbers face up and align with the numbers on the bottom tier. Snap the top tier end tabs into the upper set of slots in the end plate.
4. Bend up the opposing end plate and snap the bottom tier and then top tier end tabs into their matching slots in the end plate.

5. Bend up one side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.
6. Bend up the remaining side tier support and snap the bottom tier and then top tier side tabs into their matching slots in the side tier supports.

Submersible and works well in water baths

Autoclavable at 250° F (121°C)

Empty racks can be stacked.

Note: Do not use with liquid nitrogen.

661 Route 23 South, Wayne, NJ 07470



TEL: 973-694-0500 • FAX: 973-694-7199 • www.belart.com

918745022 - 10/15

Bel-Art – SP Scienceware assumes no obligation or liability for any advice furnished by it, or for results obtained with respect to these products.

All such advice is given and accepted at the buyer's risk.

© 2015. All Rights Reserved.

Bel-Art® – SP Scienceware® is a division of SP Industries, Inc.

